


FIG. 1

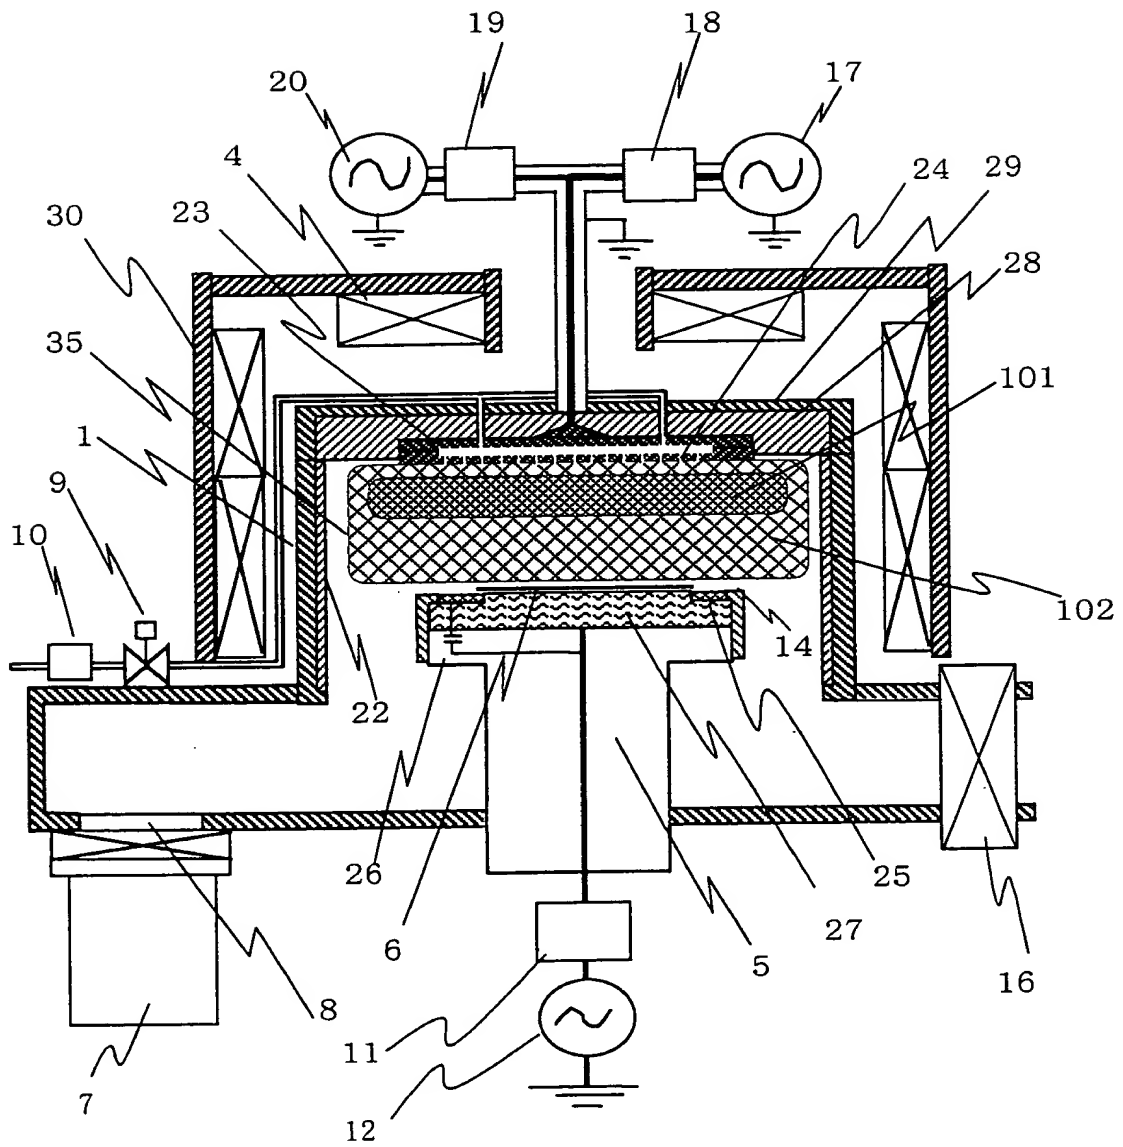

0937373.081399

FIG. 2

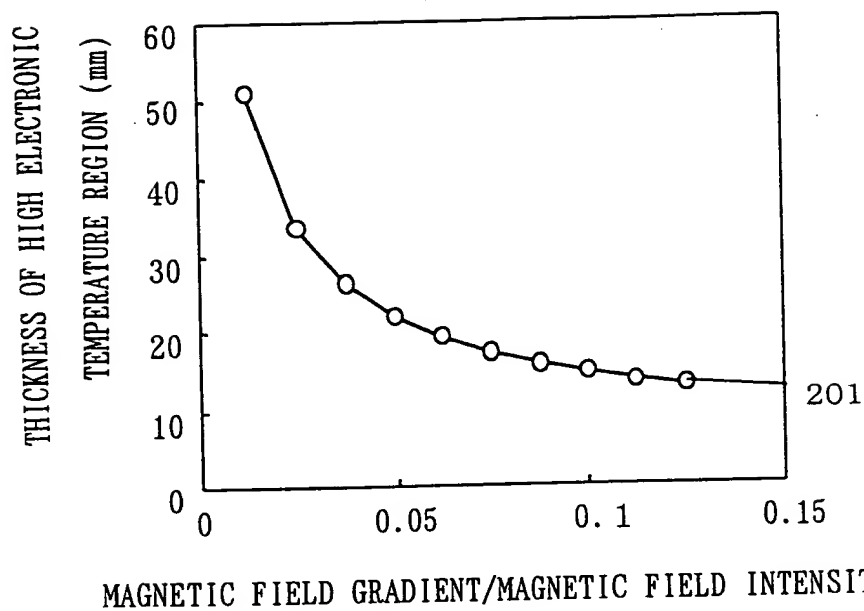


FIG. 3



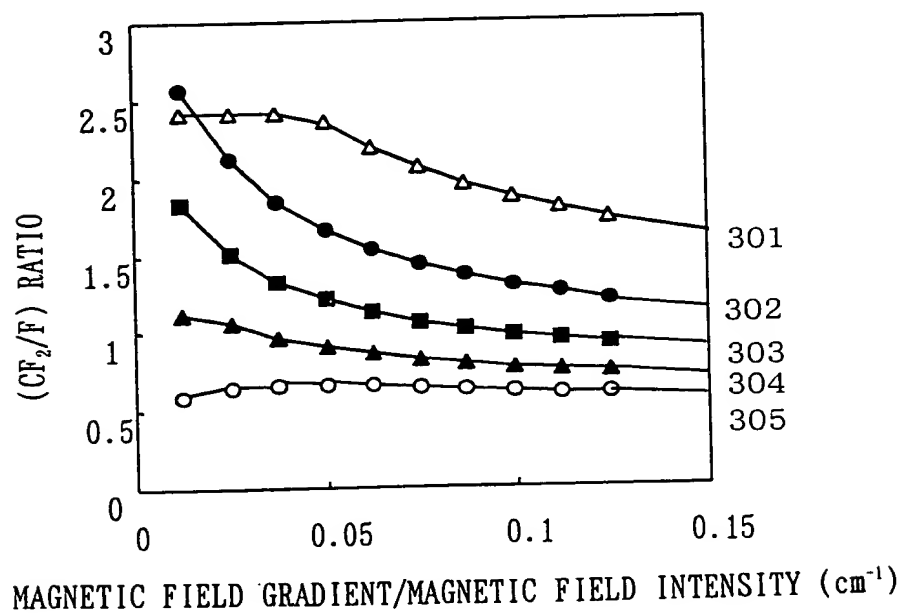


FIG. 4

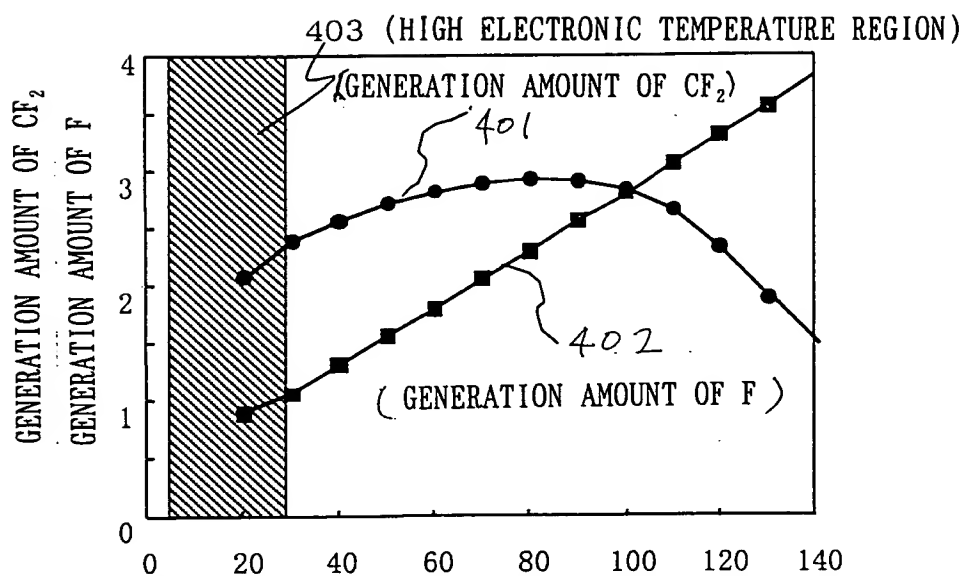

A DISTANCE BETWEEN SURFACE OF A MEMBER TO BE TREATED AND A PLANE FACING TO THE MEMBER TO BE TREATED (mm)

FIG. 5

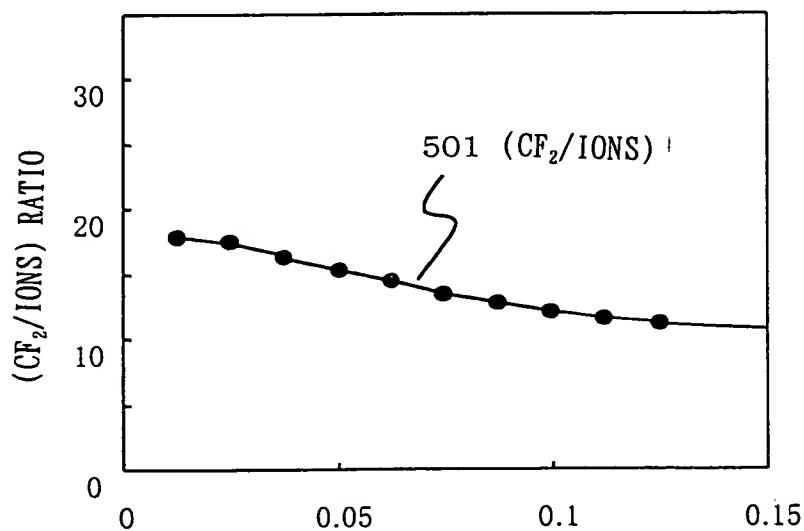

MAGNETIC FIELD GRADIENT/MAGNETIC FIELD INTENSITY (cm^{-1})

FIG. 6

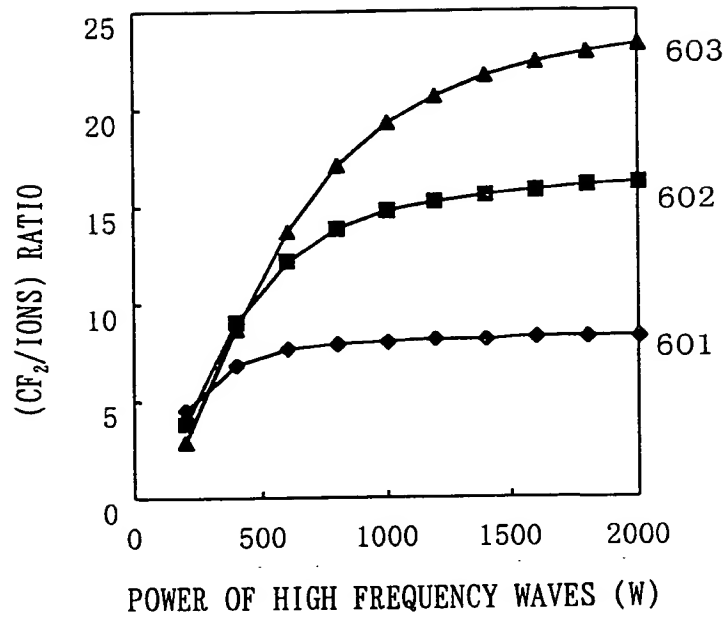


FIG. 7

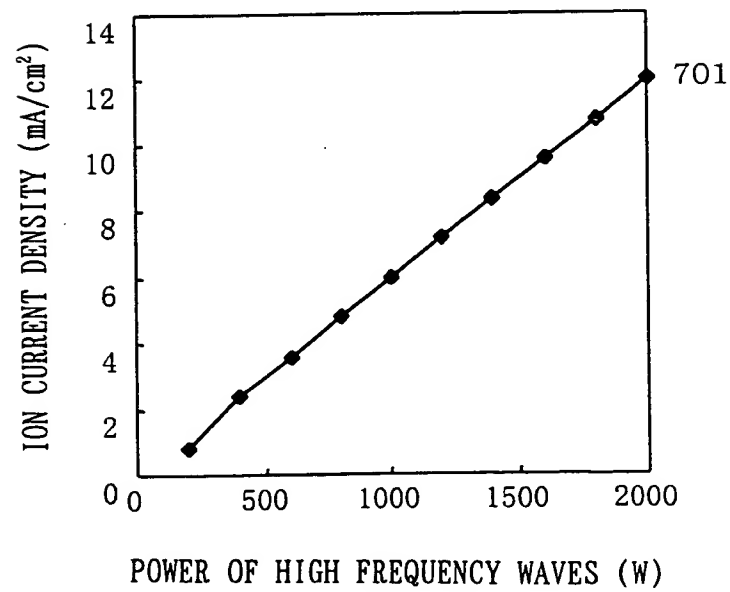


FIG. 8

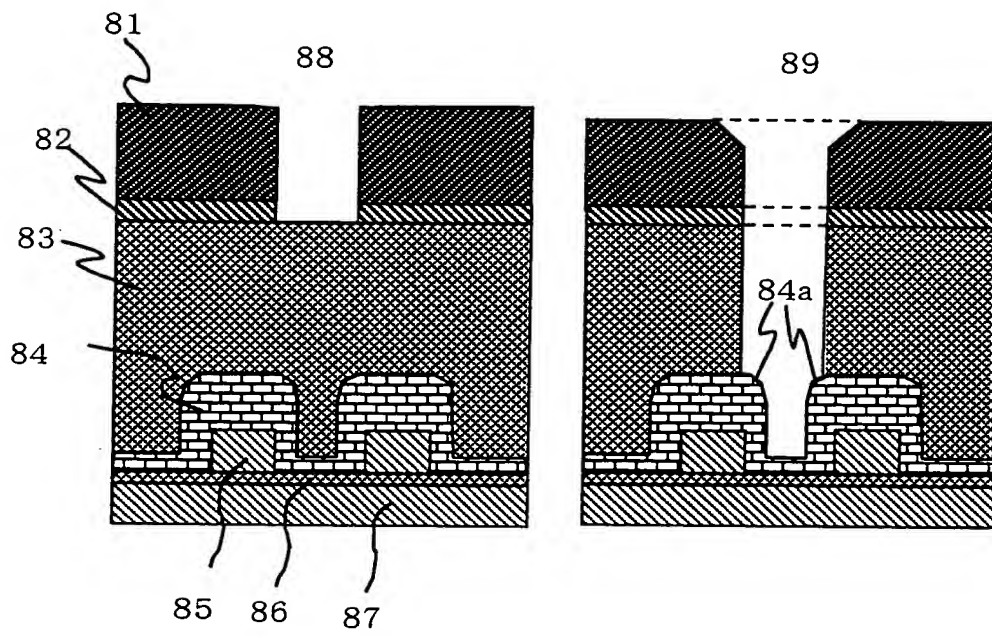


FIG. 9

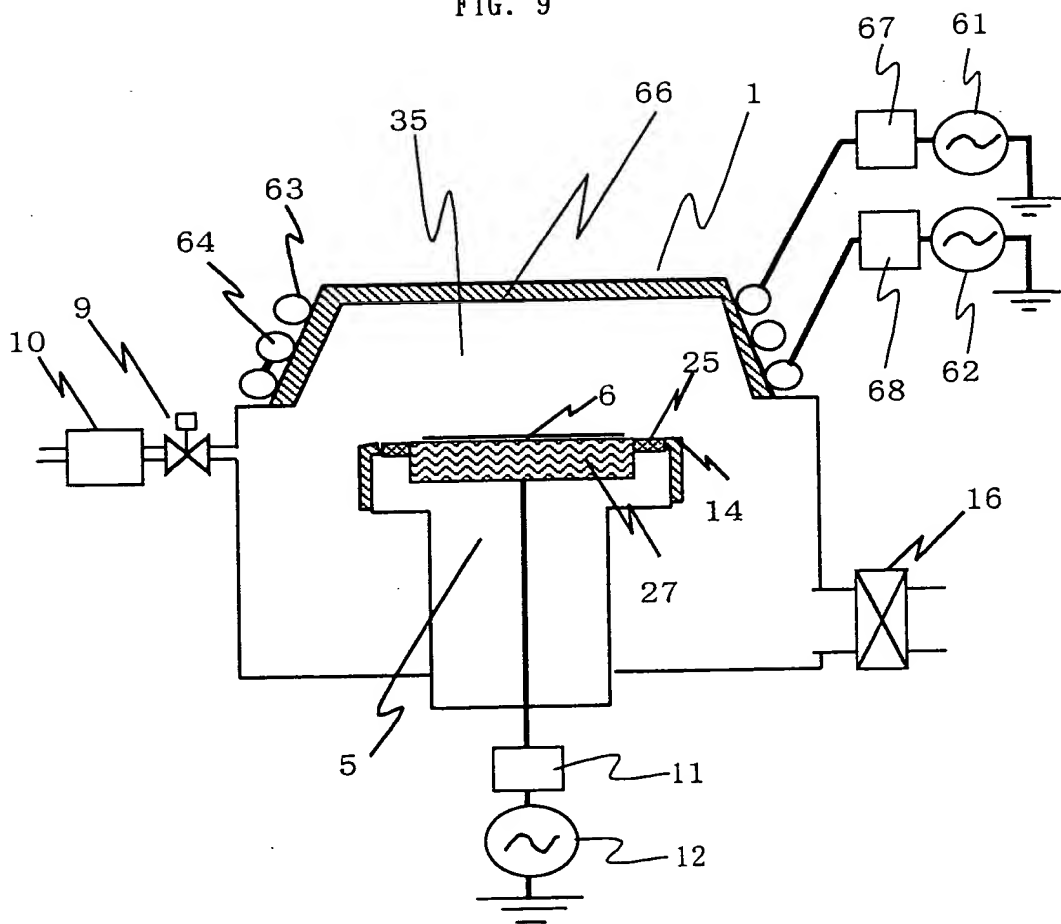


FIG. 10

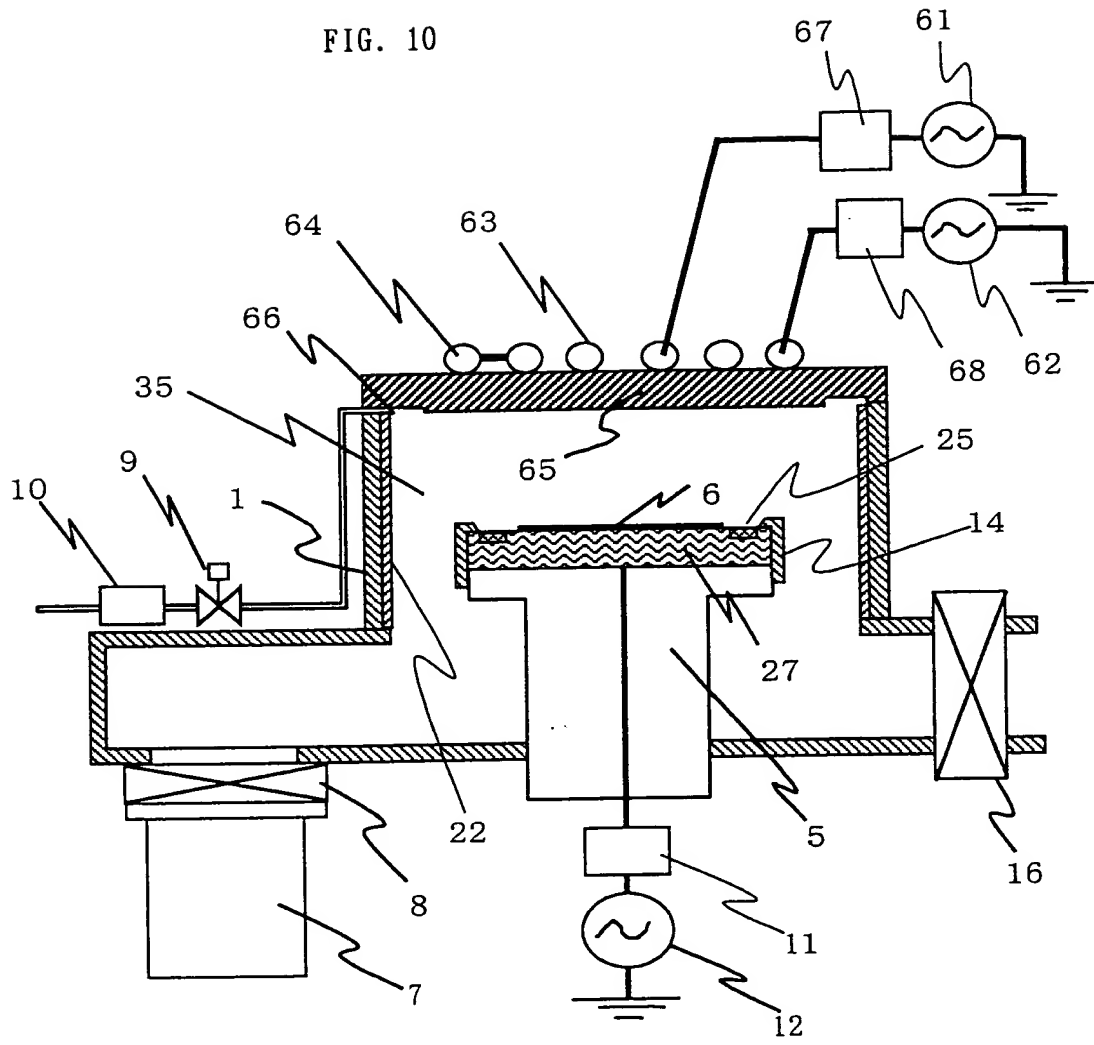


FIG. 11

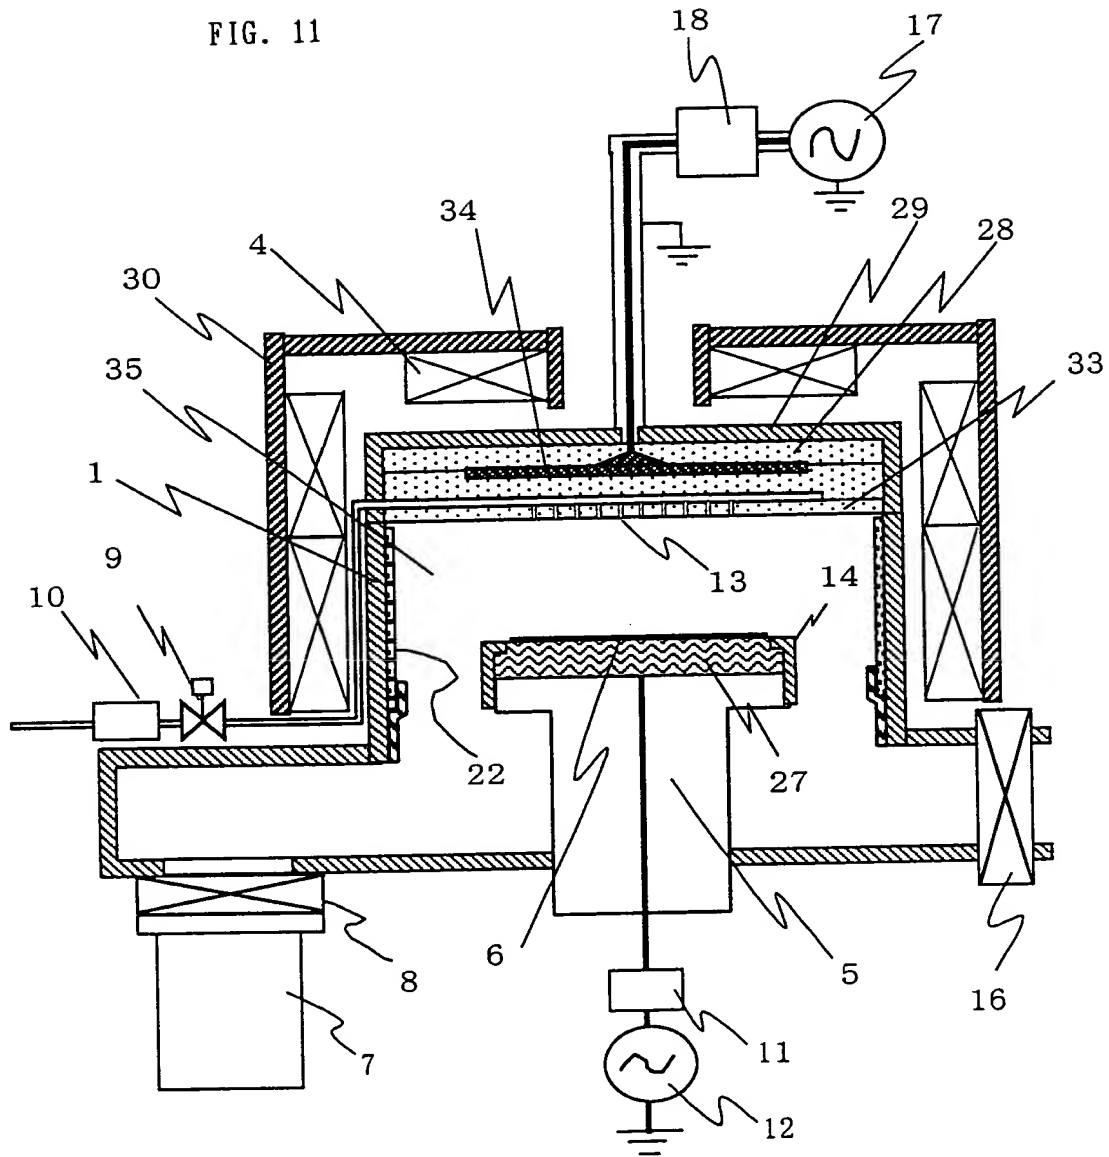


FIG. 12

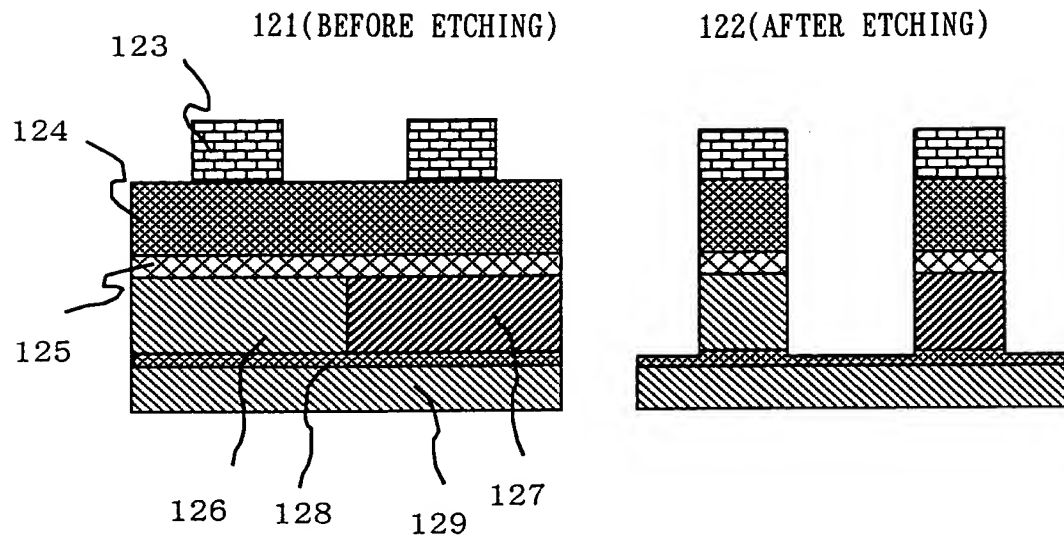


FIG. 13

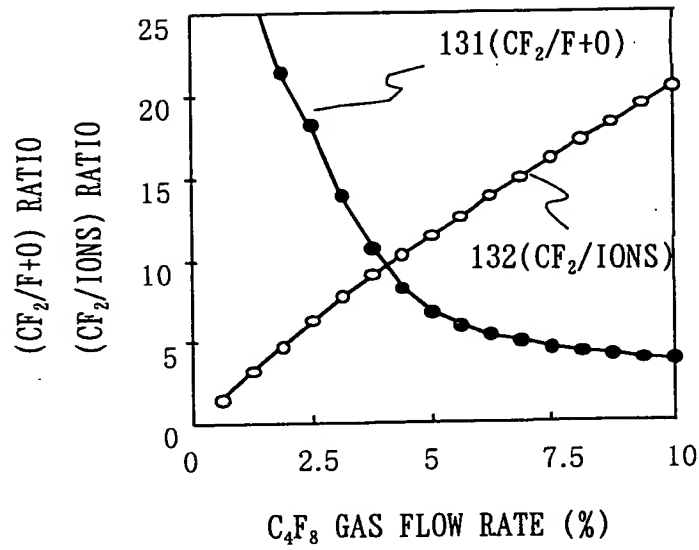


FIG. 14

